

FIG. 1

09120973 072213B

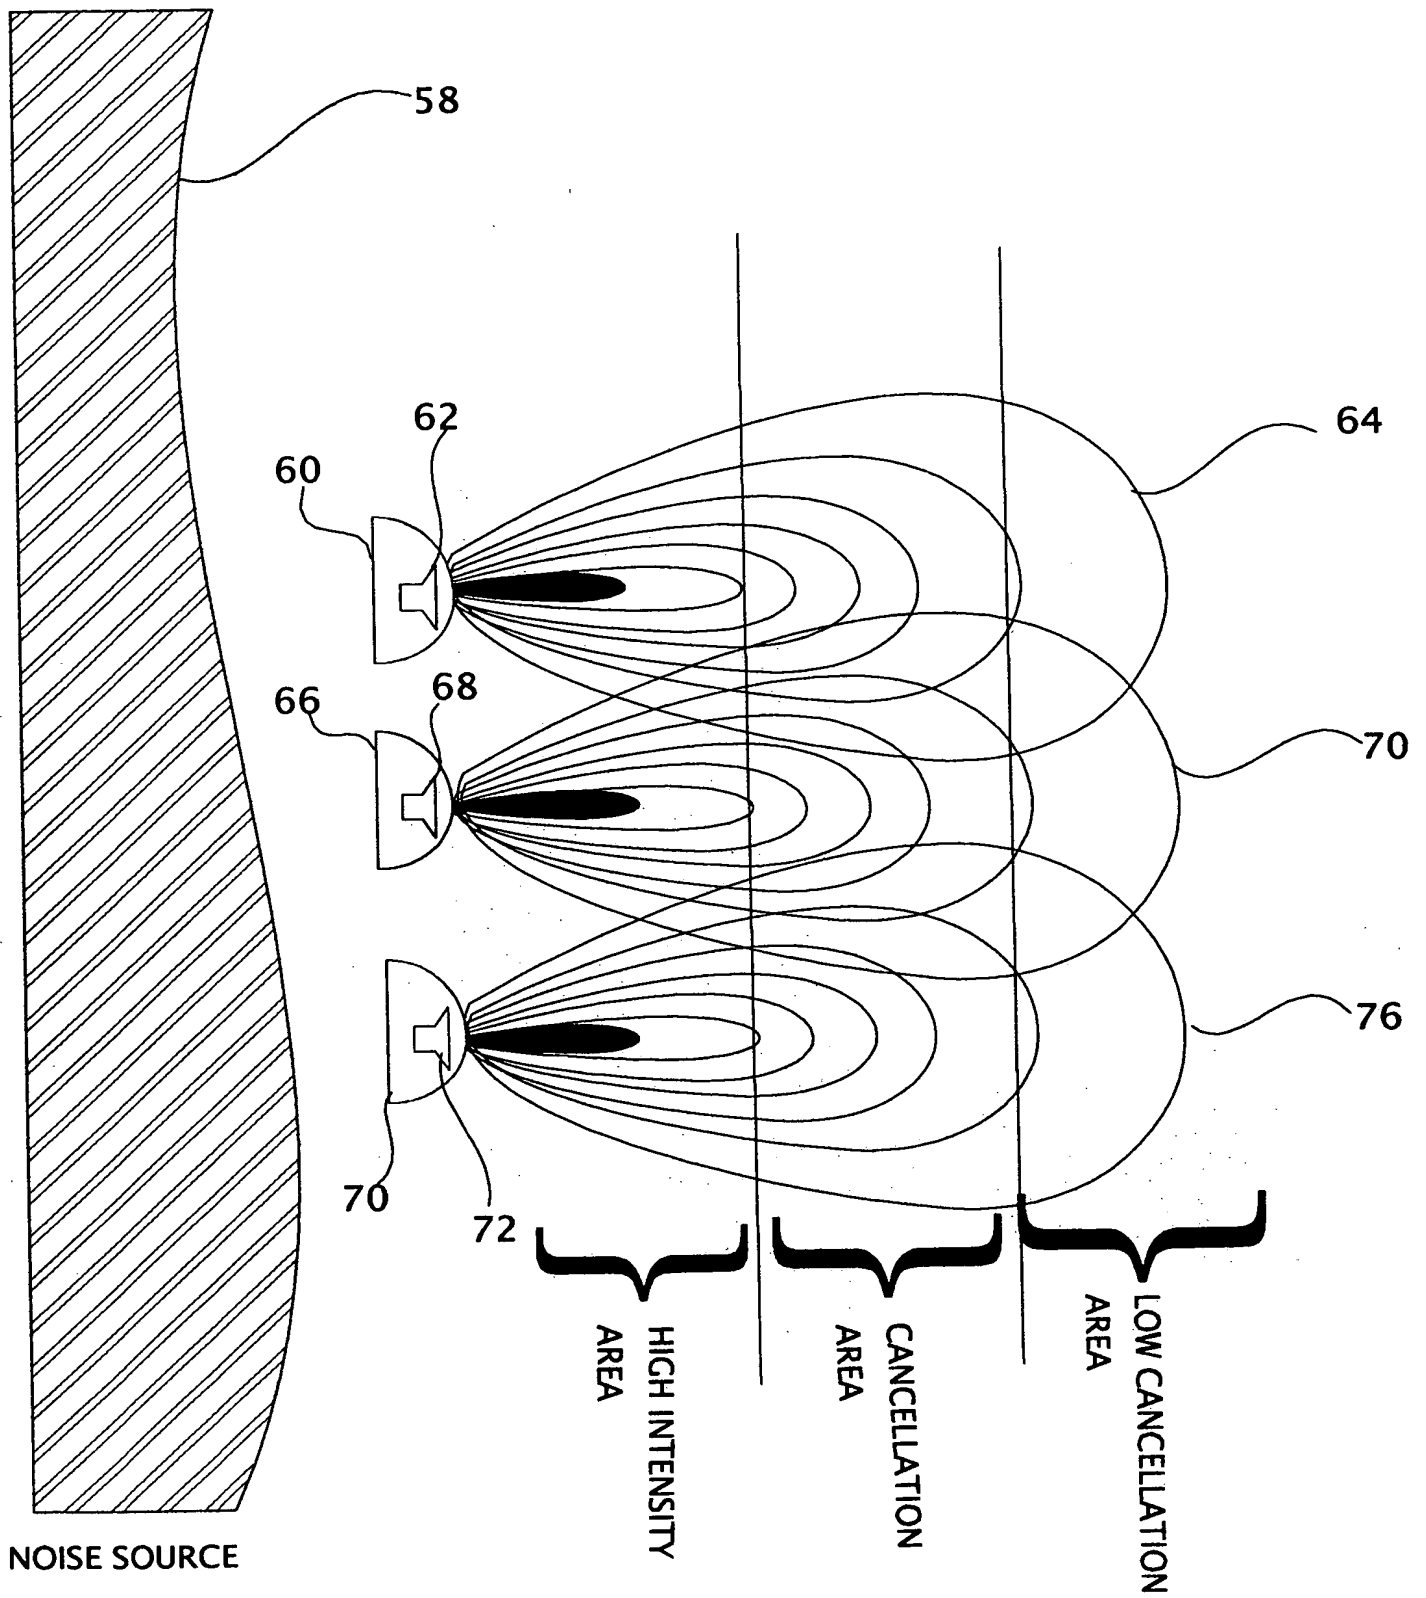


FIG. 3

2024032602150

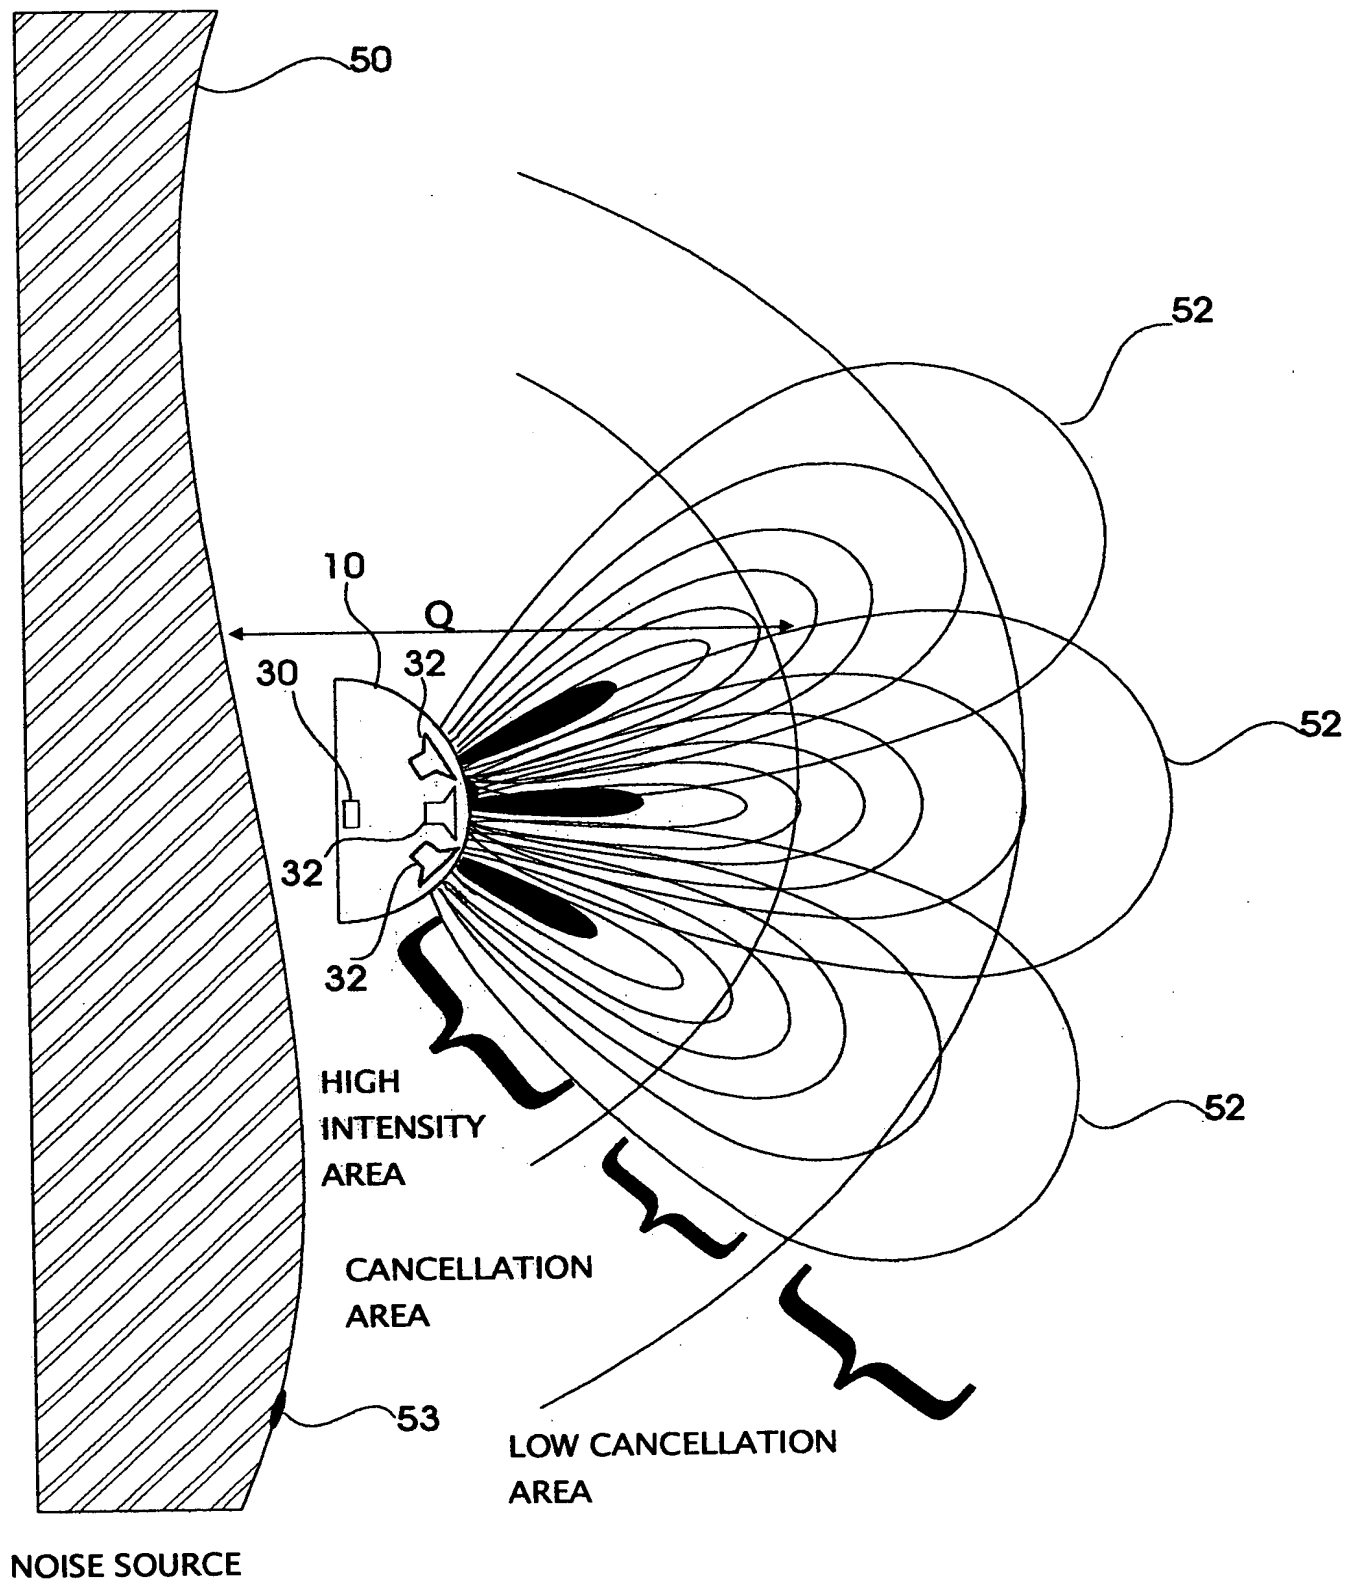


FIG. 2

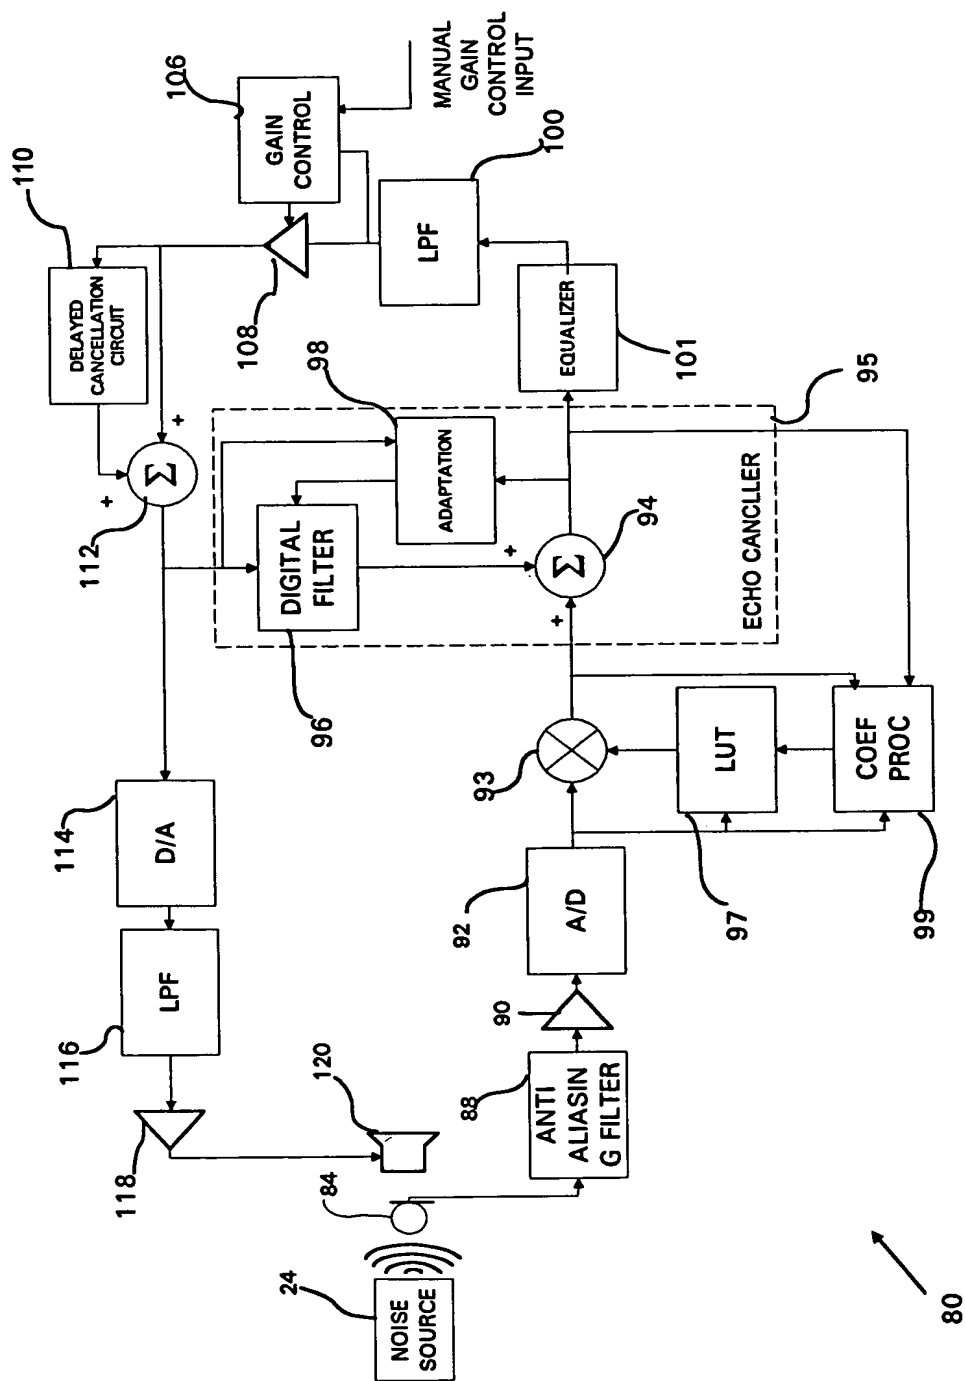


FIG. 4

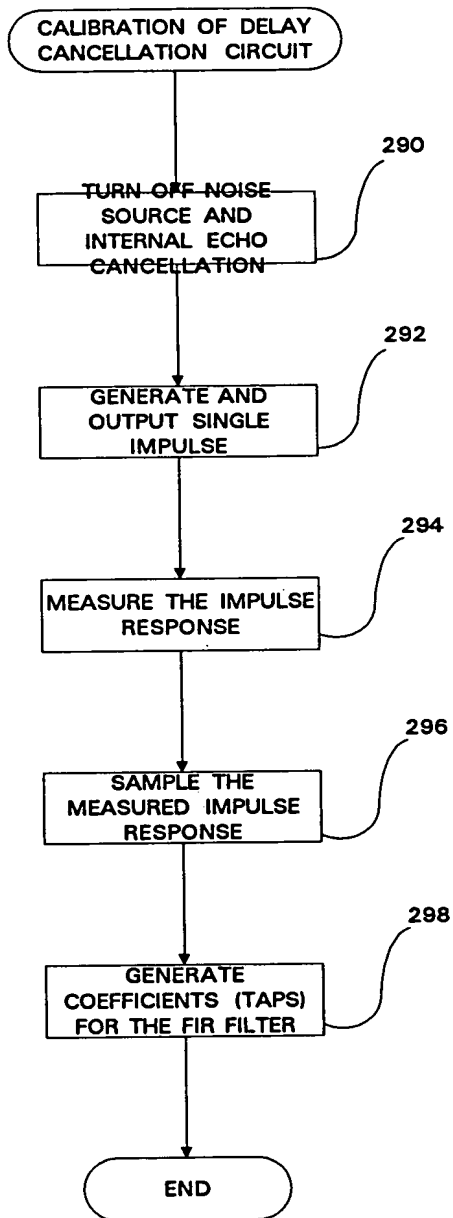


FIG. 5

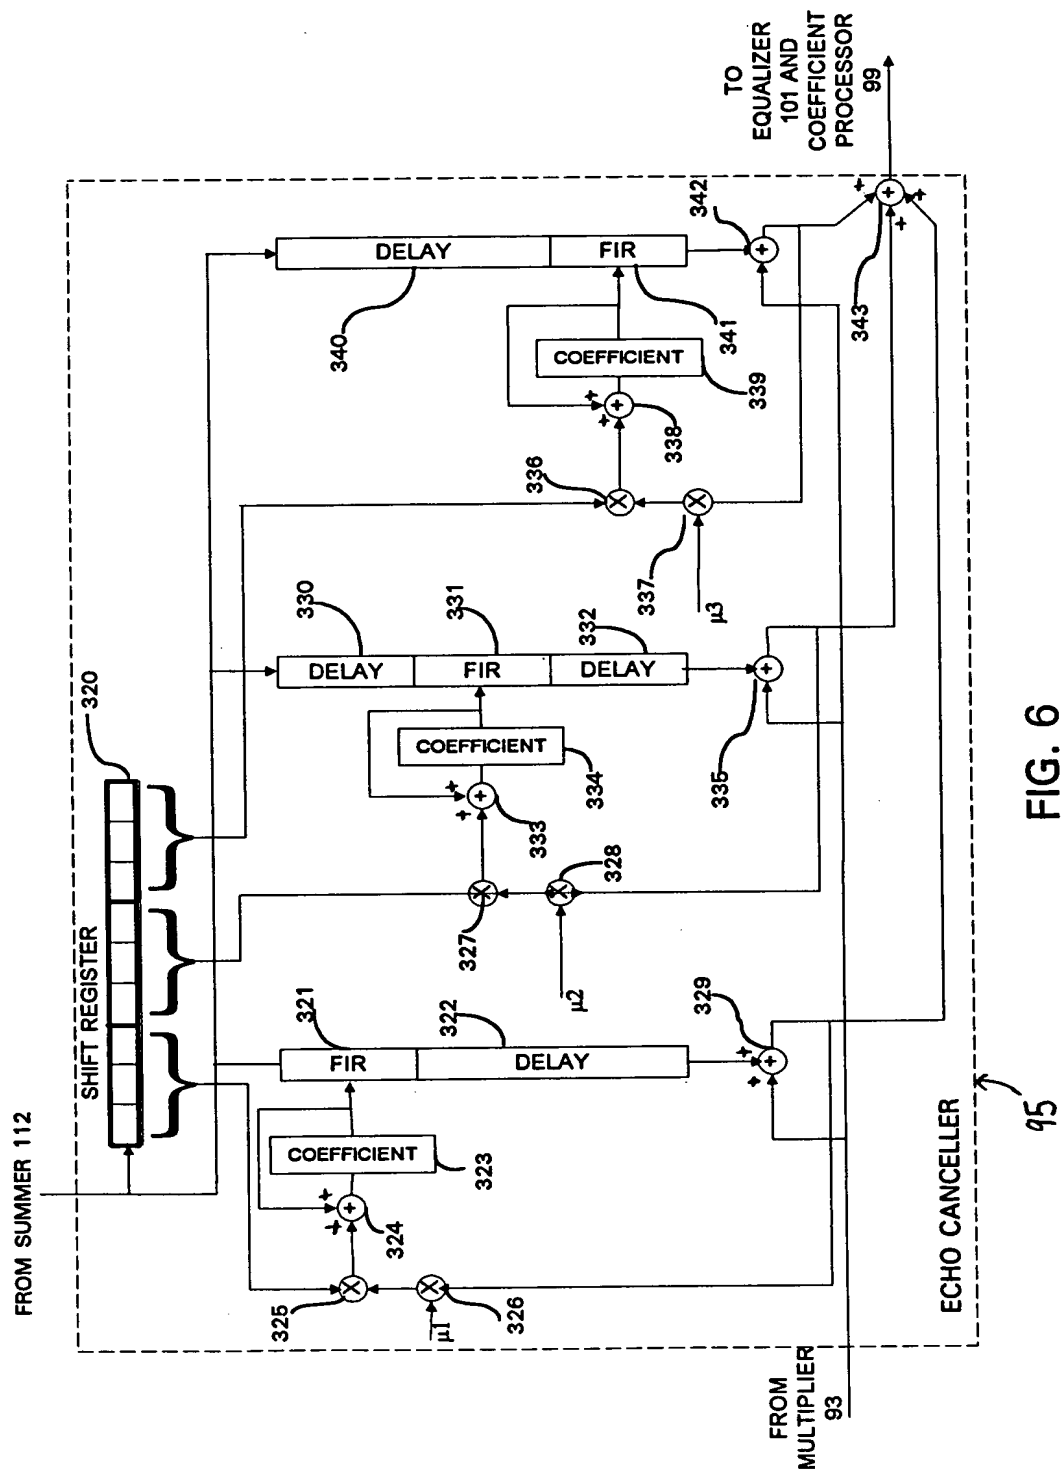


FIG. 6

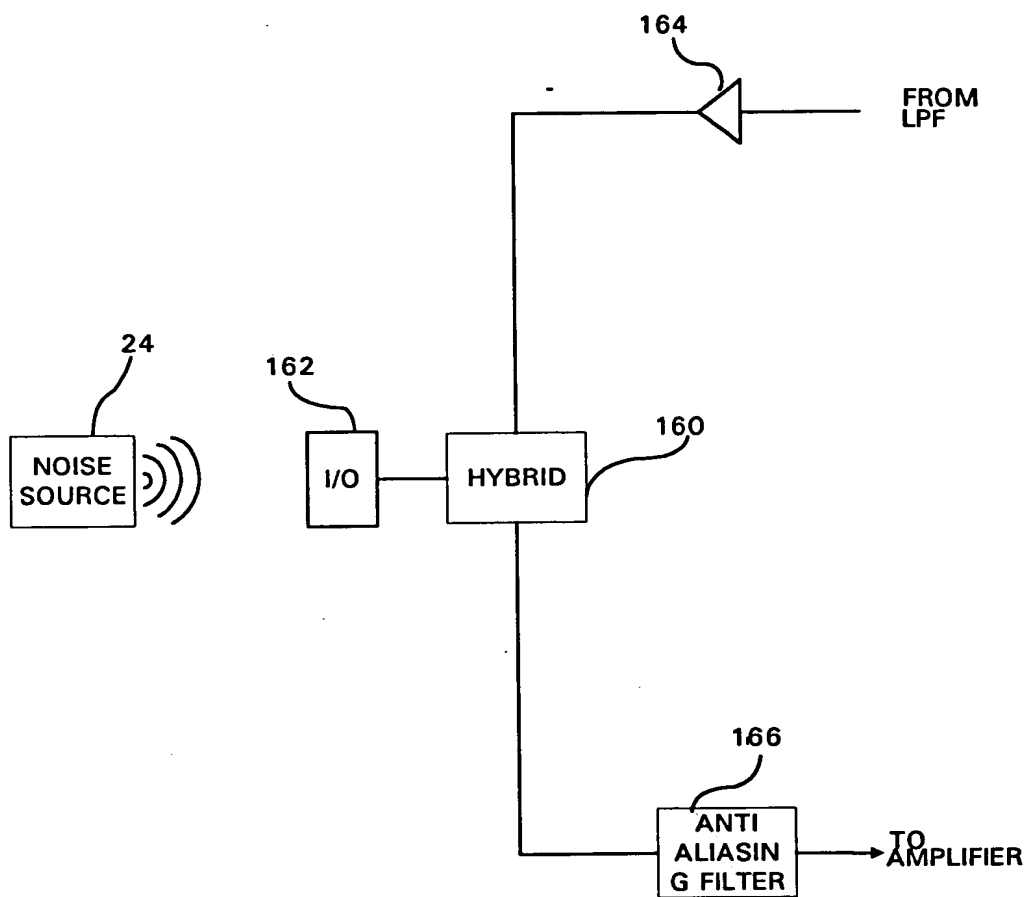


FIG . 7

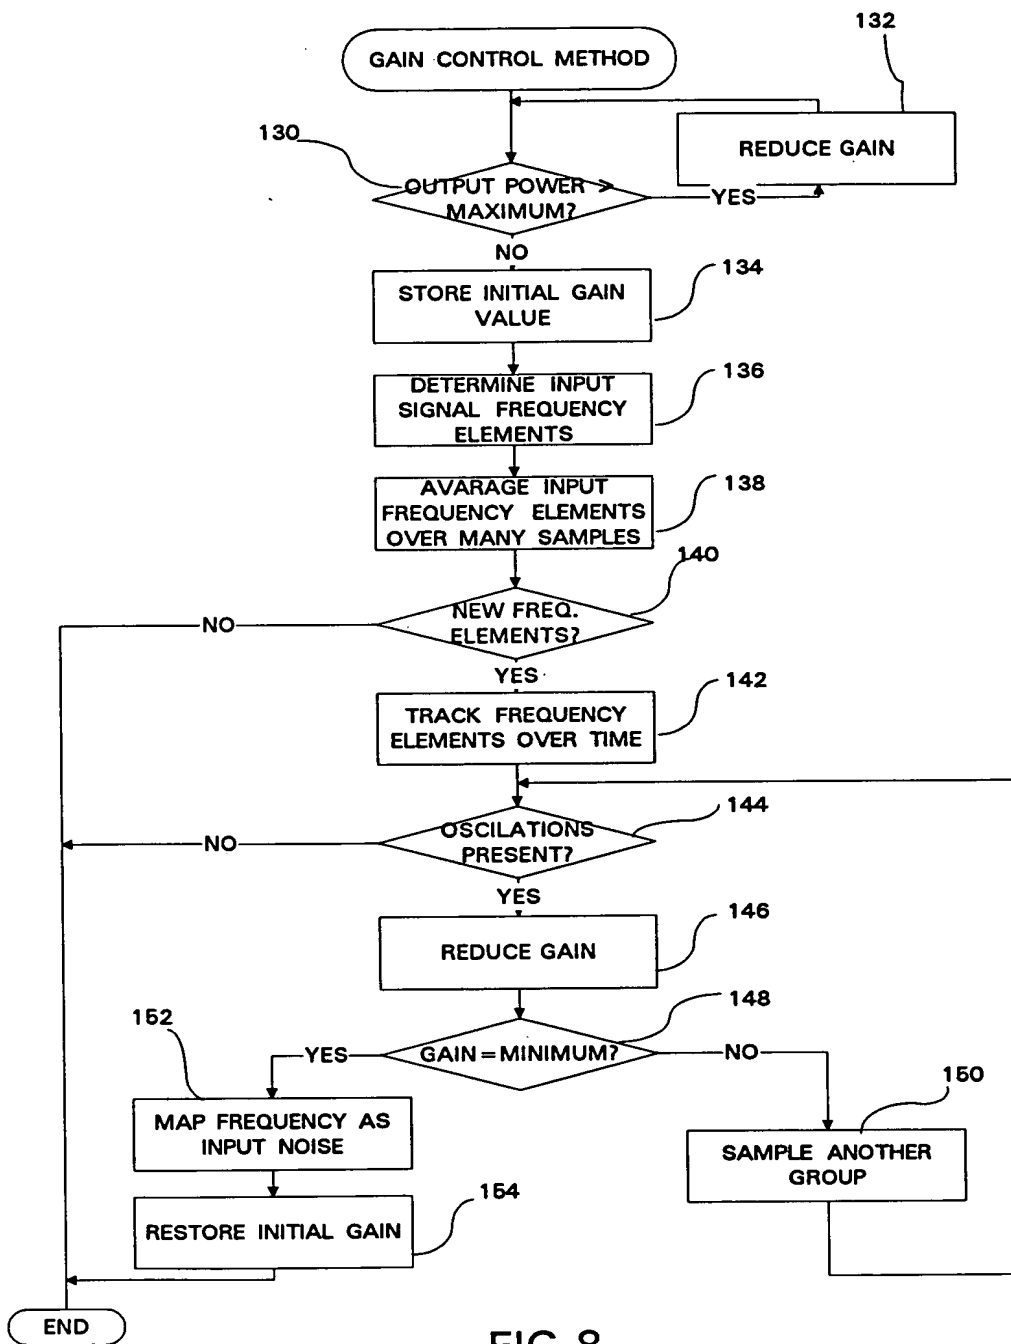


FIG.8

FIRST CALIBRATION METHOD
WITH ECHO CANCELLATION

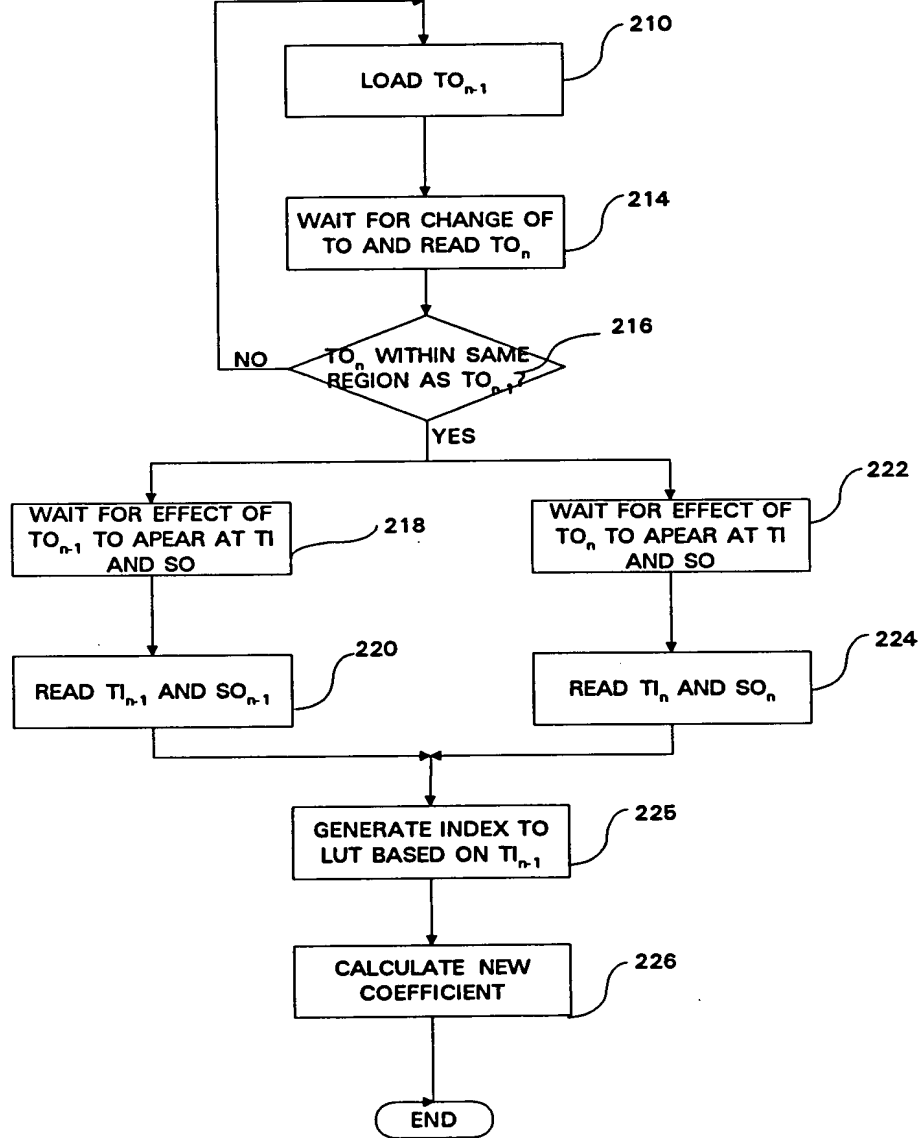


FIG. 9

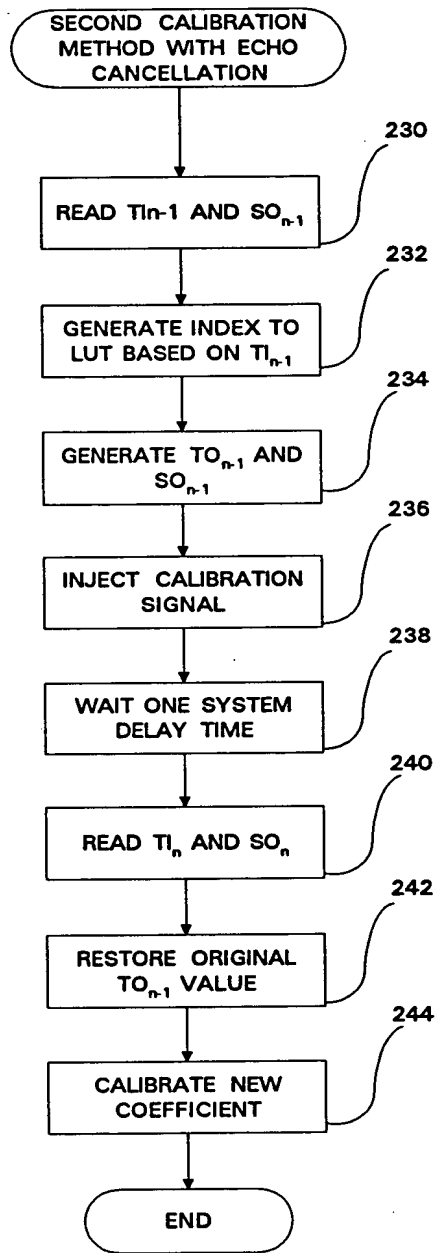


FIG. 10

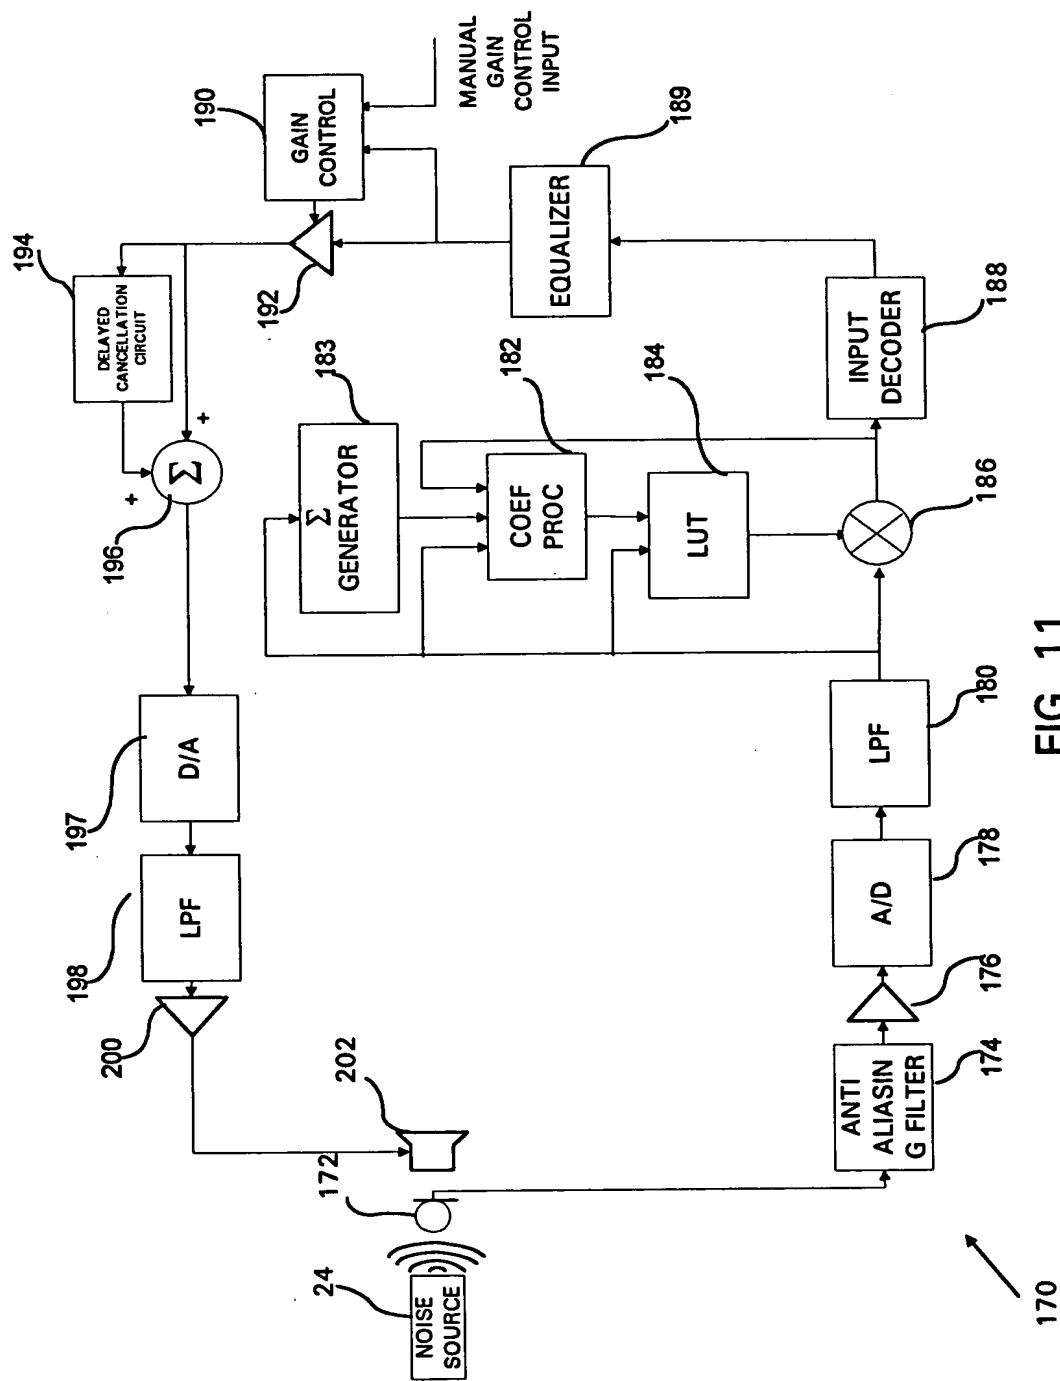


FIG. 11

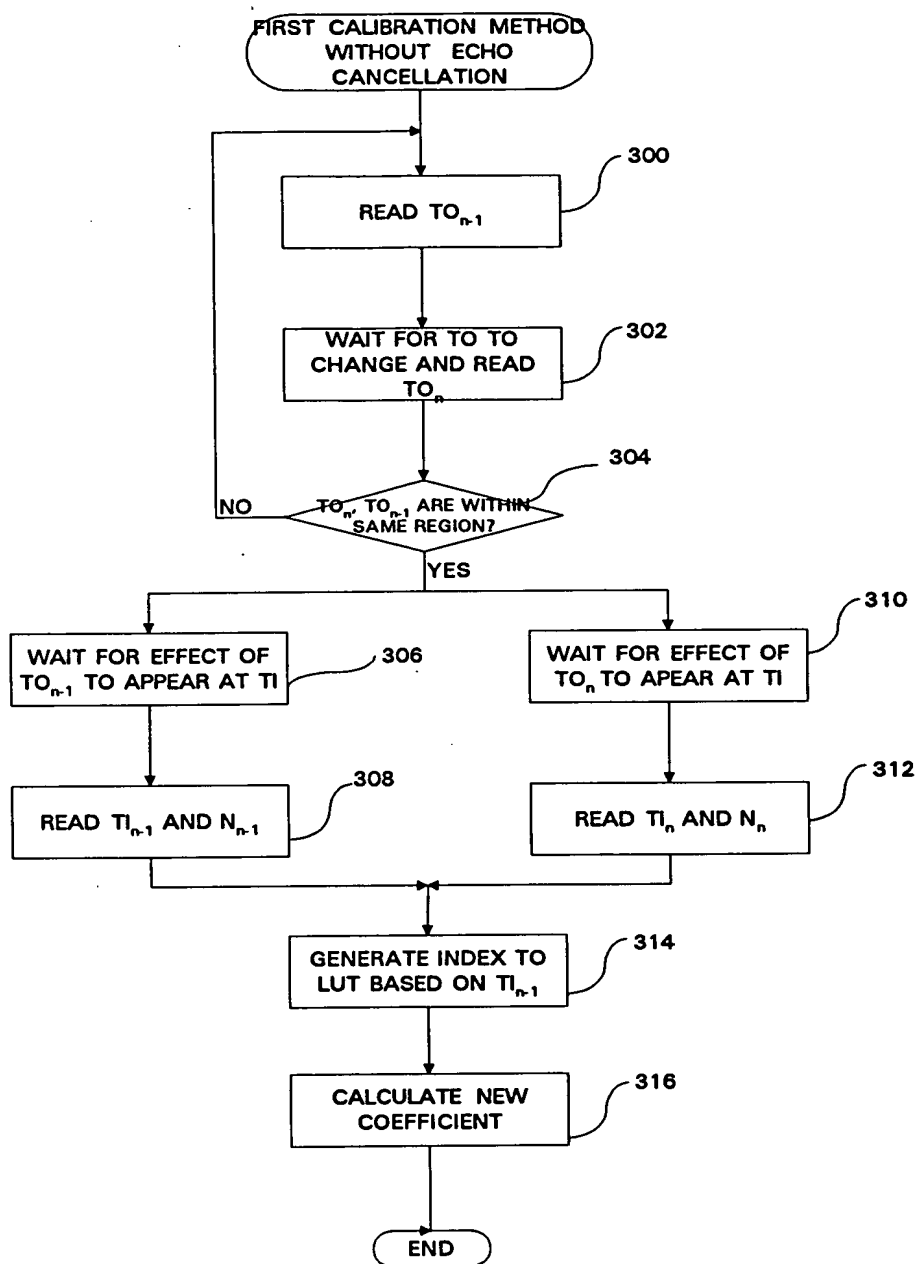


FIG. 12

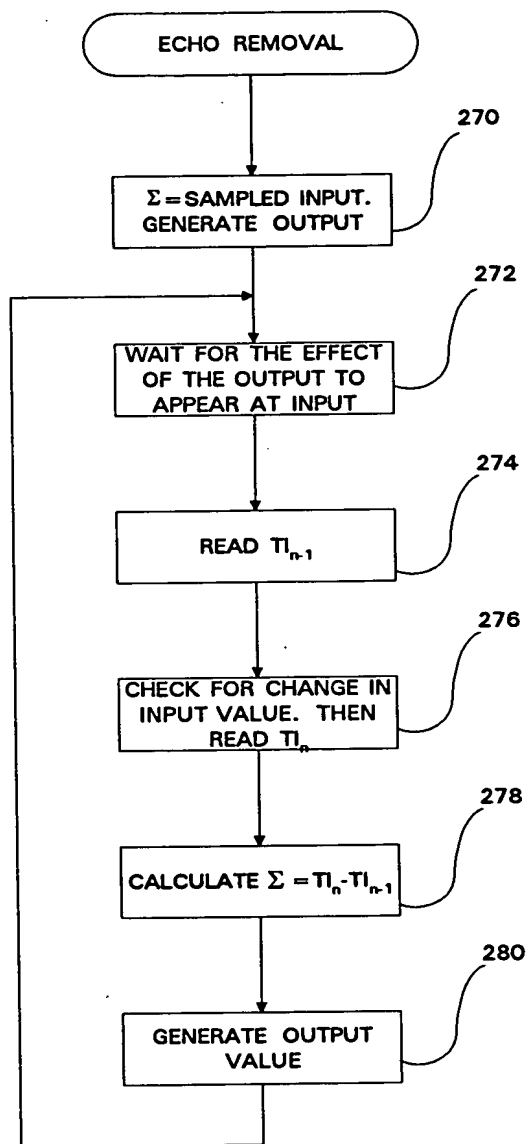


FIG. 13

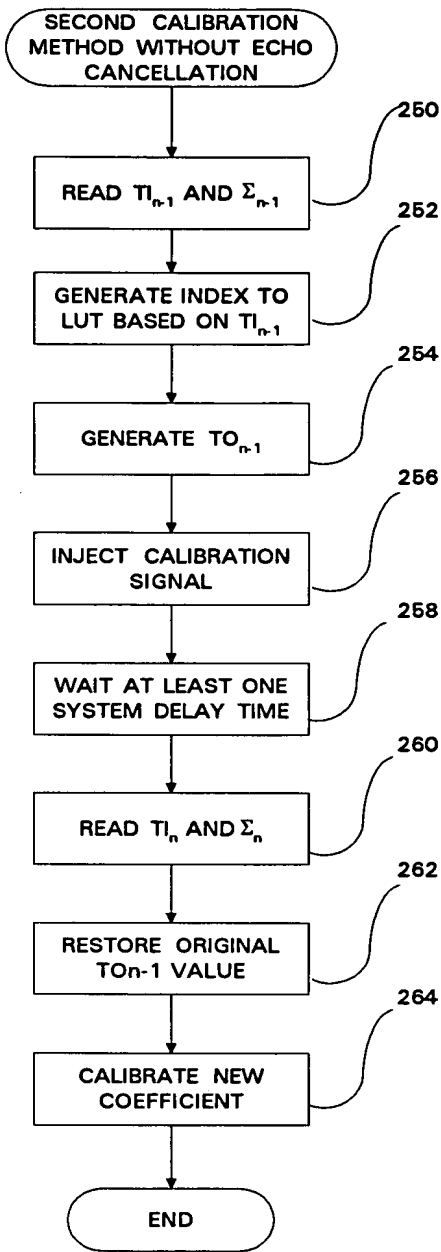


FIG. 14